

## Artificial Eye Measurement Performed on 13-Dec-2013

Artificial eye measurements in three trials. The duration of each trial is 10 seconds.

	Trial 1	Trial 2	Trial 3
Mean_Hor	0.1380	0.1395	0.1411
Mean_Ver	0.0486	0.0485	0.0481
Std_Hor	0.0017	0.0018	0.0018
Std_Ver	0.0016	0.0016	0.0016

Figure 1: Mean and standard deviation in horizontal and vertical axis.

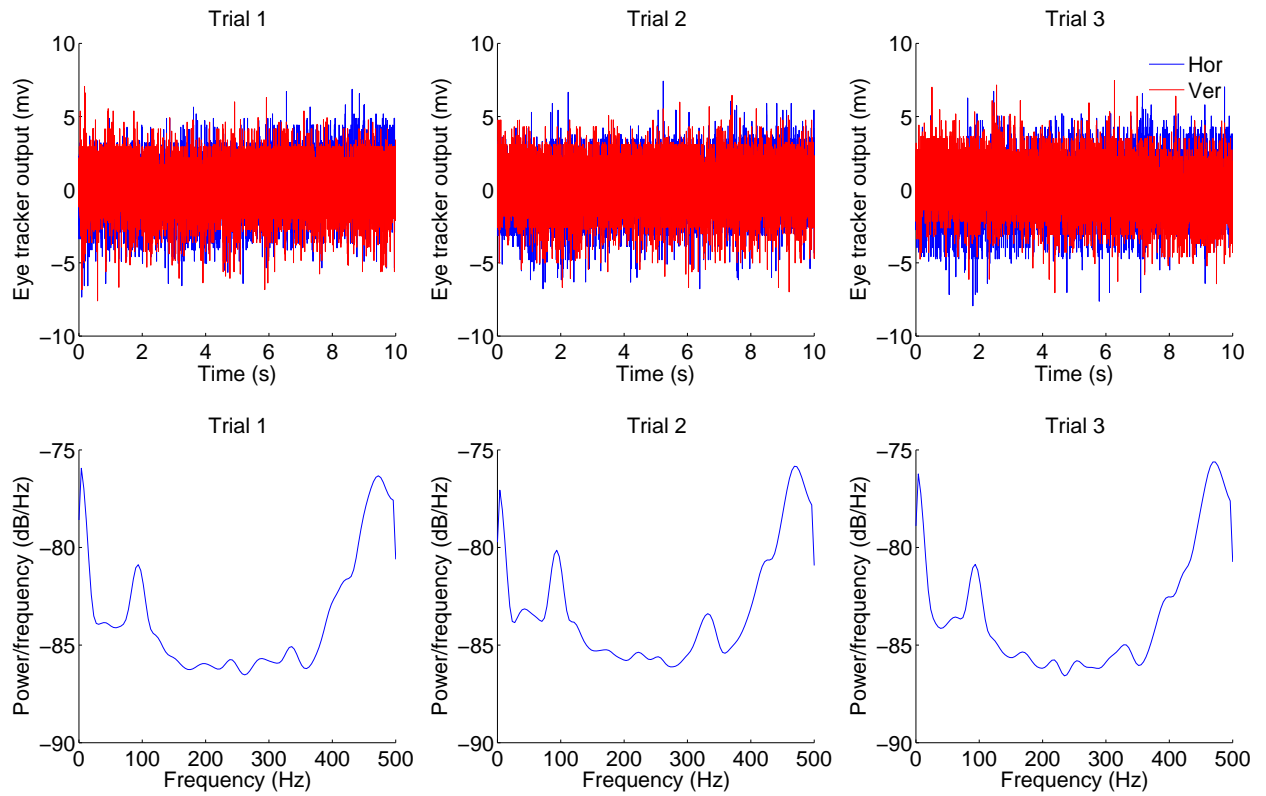


Figure 2: Top row represents the eye tracker output in horizontal and vertical axis for each trial. the bottom row are the PSD of the output calculated by Welch method. Each column refers to one trial.