

## Artificial Eye Measurement Performed on 20-Dec-2013

Artificial eye measurements in three trials. The duration of each trial is 10 seconds.

	Trial 1	Trial 2	Trial 3
Mean_Hor	0.1439	0.1458	0.1477
Mean_Ver	0.0516	0.0515	0.0519
Std_Hor	0.0021	0.0020	0.0020
Std_Ver	0.0014	0.0015	0.0015

Figure 1: Mean and standard deviation in horizontal and vertical axis.

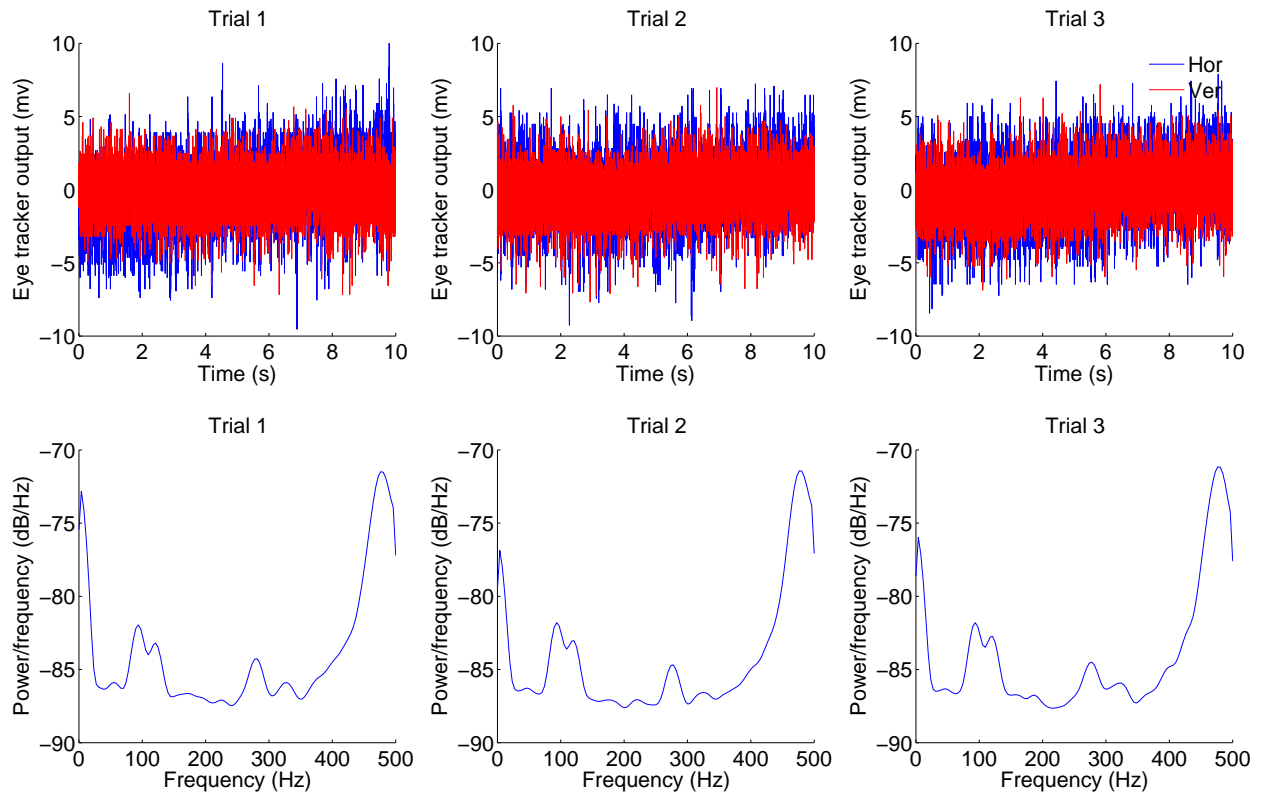


Figure 2: Top row represents the eye tracker output in horizontal and vertical axis for each trial. the bottom row are the PSD of the output calculated by Welch method. Each column refers to one trial.