

Artificial Eye Measurement Performed on 29-Jan-2014

Artificial eye measurements in three trials. The duration of each trial is 10 seconds.

	Trial 1	Trial 2	Trial 3
Mean_Hor	0.15498	0.15476	0.15473
Mean_Ver	0.01753	0.01759	0.01769
Std_Hor	0.00124	0.00123	0.00125
Std_Ver	0.00091	0.00087	0.00086

Figure 1: Mean and standard deviation in horizontal and vertical axis.

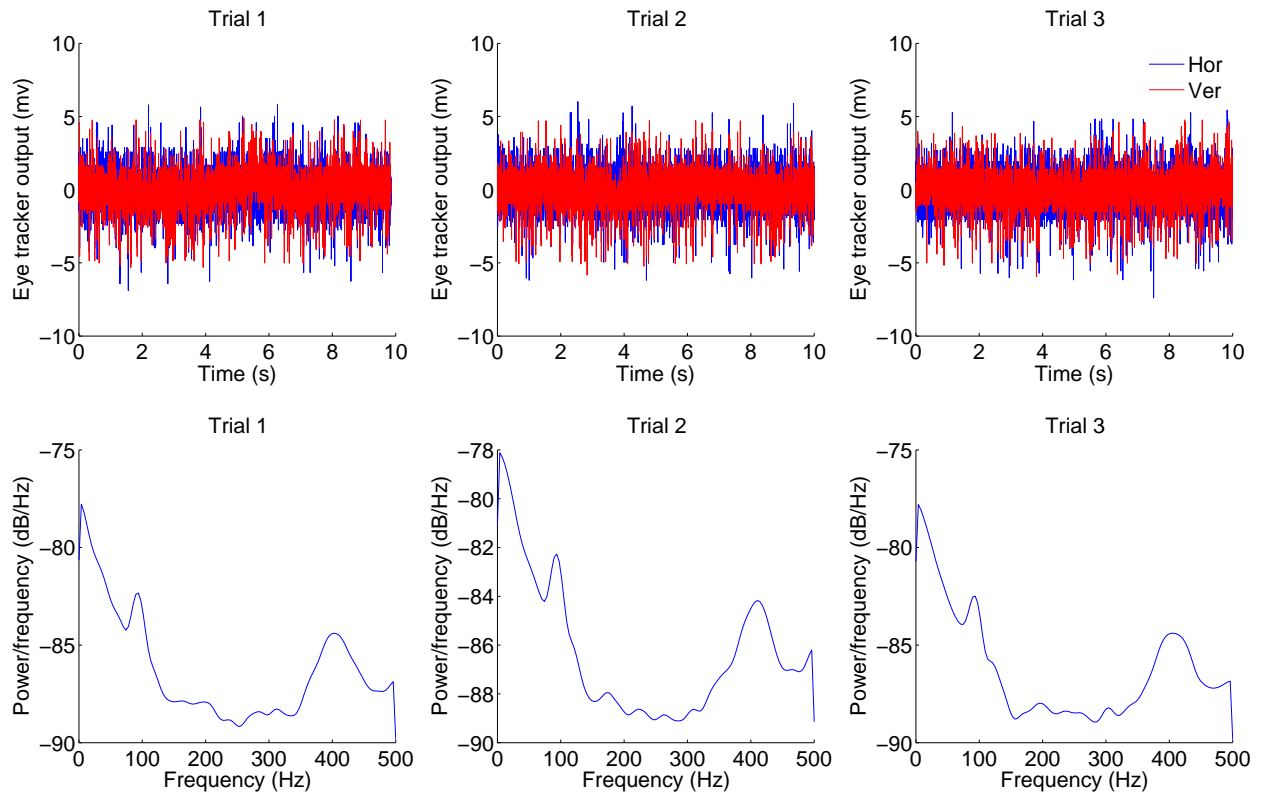


Figure 2: Top row represents the eye tracker output in horizontal and vertical axis for each trial. the bottom row are the PSD of the output calculated by Welch method. Each column refers to one trial.